

# Human GM-CSF ELISA Kit

**Please read the manual carefully before use.**

**Cat. No.** NE105


**Storage:** at 2~8°C in the dark for one year.



## Description

Human granulocyte-macrophage colony-stimulating factor, also known as GM-CSF, or CSF-2, is a monomeric glycoprotein secreted by a variety of activated immune cells, mesenchymal cells and epithelial cells. The amino acid sequence homology of mature human GM-CSF with mouse and rat GM-CSF is 54% and 63%, respectively. GM-CSF has multiple biological functions, such as the ability to stimulate the differentiation of CD34+ stem cell precursors into monocytes, neutrophils and eosinophils; it can act as a chemokine for neutrophils and dendritic cells. GM-CSF is also involved in the autoimmune response mediated by Th1 and Th17 cells and is related to the inflammatory activation of dendritic cells, microglia, alveolar macrophages and eosinophils. In addition, GM-CSF regulates tumor cell proliferation, invasion and metastasis through immune-dependent and independent pathways.

This kit uses the Sandwich Enzyme-Linked Immunosorbent Assay (ELISA) to measure the amount of GM-CSF in human serum, plasma, and cell culture supernatant. The ELISA microplate in the kit is precoated with a high-affinity anti-human GM-CSF antibody. The standard or test sample and a biotin-labeled anti-human GM-CSF detection antibody are added to the microplate wells at the same time. After incubation, GM-CSF present in the sample will be bound specifically to the precoated antibody and the detection antibody. After washing, a horseradish peroxidase-labeled streptavidin (Streptavidin-HRP) is added to the microplate wells and incubated. Biotin and streptavidin on the detection antibody produces the "coated antibody-human GM-CSF protein-detection antibody-Streptavidin-HRP" immune complex through high-strength non-covalent binding. After washing again, the chromogenic substrate TMB is added to the wells. HRP catalyzes the TMB substrate to create blue coloration, with intensity positively correlated with the concentration of GM-CSF in the sample. The reaction is stopped by adding stop solution, and the absorbance is measured at 450 nm (reference wavelength 570-630 nm). A standard curve is drawn to calculate the concentration of GM-CSF in the sample based on the absorbance value. This kit is highly specific, has high detection sensitivity and is convenient to use.

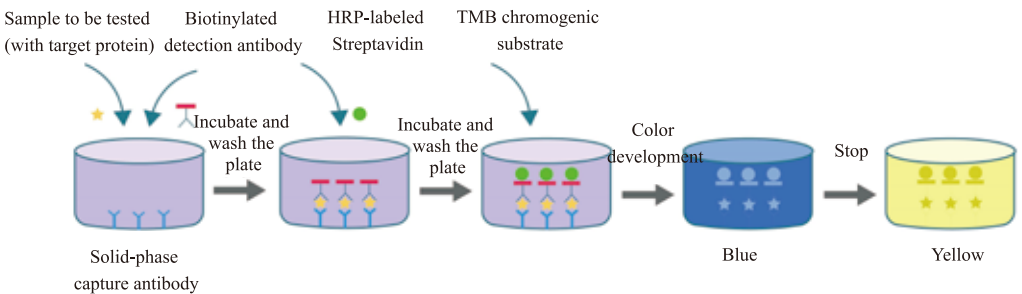

Principle of sandwich ELISA with antibody pairs

## Suitable Sample Types

Cell culture supernates, serum, plasma, etc.



### Kit Contents

Component	NE105-01	Storage
Human GM-CSF Antibody Precoated ELISA Plate	96 T	at 2~8°C
Human GM-CSF Standard	2 bottles	at 2~8°C
100× Human GM-CSF Detection Antibody	60 µl/test	at 2~8°C
Standard & Sample & Antibody Diluent	25 ml/bottle	at 2~8°C
100×Streptavidin-HRP	120 µl/test	at 2~8°C in the dark
Streptavidin-HRP Diluent	15 ml/bottle	at 2~8°C
20× Wash Buffer	50 ml/bottle	at 2~8°C
TMB Chromogenic Substrate	12 ml/bottle	at 2~8°C in the dark
Stop Solution	6 ml/bottle	at 2~8°C
Plate Sealers	4 pieces	

Note: The kit can be stored at 2~8°C for 1 month when it was opened; please use the unopened kit within 1 year.

### Self-prepared Regents and Equipment

1. Microplate reader: at a main wavelength of 450 nm, a reference wavelength of 620 nm.
2. Deionized water.
3. EP tubes, pipettes, tips, graduated cylinders, etc.
4. Microplate shaker.
5. Automatic plate washer or 8-channel manual plate washer or multi-channel pipette.

### Sample Collection

1. Cell culture supernatant: Collect the cell culture supernatant and centrifuge it at  $300 \times g$  for 10 minutes at 4°C. Aliquot the supernatant into EP tubes and store at -20°C. Avoid repeated freeze-thaw cycles. For detection within 24 hours, it can be stored at 2~8°C.
2. Serum: After the blood has clotted for 30 minutes at room temperature, centrifuge it at  $1000 \times g$  for 10 minutes at 4°C. Then, divide the supernatant into EP tubes and store at -20°C. Avoid repeated freeze-thaw cycles. For detection within 24 hours, it can be stored at 2~8°C.
3. Plasma: EDTA or sodium citrate is recommended as anticoagulants. Collect the whole blood into blood collection tubes containing anticoagulant and mix it. After placing it for at least 20 minutes at room temperature, centrifuge it at  $1000 \times g$  for 10 minutes at 4°C. Aliquot the supernatant into EP tubes and store it at -20°C. Avoid repeated freeze-thaw cycles. For detection within 24 hours, it can be stored at 2~8°C.

Note: Serum and plasma samples with hemolysis and hyperlipidemia may affect the accuracy of test results and should be avoided.

### Sample Dilution


1. Serum/plasma samples need to be diluted 2-fold with standard & sample & antibody diluent, for example: 100 µl serum + 100 µl standard & sample & antibody diluent.
2. If the positive value of the cell culture supernatant sample is within the range of the curve, it does not need to be diluted with the diluent, and can be directly detected with the original solution; if the positive value exceeds the range of the curve, it needs to be diluted to the curve range with the diluent for detection. The concentration should be multiplied by the corresponding dilution factor when calculating.
3. It is recommended to perform a pre-experiment to determine the dilution factor before the formal experiment.



### Working Solution Preparation

Bring all reagents to room temperature before use. If crystals appear in the 20× Wash Buffer, put them in a water bath at 37°C until all the crystals have dissolved.


- 1×Human GM-CSF Detection Antibody:** Spin and centrifuge the tube before use to collect the liquid on the tube wall at the bottom. Dilute 100× human GM-CSF detection antibody to 1× working concentration with standard & sample & antibody diluent according to the amount required for the current experiment. Use within 15 minutes after preparation.
- 1×Streptavidin-HRP:** Spin and centrifuge the tube before use to collect the liquid on the tube wall at the bottom. Dilute 100× Streptavidin-HRP to 1×working concentration with Streptavidin-HRP diluent according to the amount required for the experiment. Use within 15 minutes after preparation.
- 1×Wash Buffer:** Dilute the 20×washing solution to 1×working concentration with deionized water according to the amount required for the current experiment. After preparation, it can be stored at 2–8°C for 30 days.
- Dissolve Human GM-CSF Standard:** Dissolve the lyophilized standard with the corresponding volume of standard & sample & antibody diluent according to the dissolution volume indicated on the standard label. The concentration of the reconstituted standard is 5000 pg/ml. Please use the redissolved standard within 30 minutes.
- Standard Gradient Dilution:** Dilute the redissolved standard 10 times with Standard & Sample & Antibody Diluent, take 60 µl of the reconstituted standard, add it to 540 µl standard & sample & antibody diluent, mix well, record it as a tube 1, and the concentration of tube 1 at this time is 500 pg/ml; then perform a 2-fold gradient dilution according to the figure below, and add 300 µl of standard & sample & antibody diluent to tubes 2-7 respectively; take 300 µl of the liquid from the No. 1 tube and add it to the No. 2 tube. At this time, the concentration of the No. 2 tube is 250 pg/ml. After mixing, take 300 µl and add it to the No. 3 tube. At this time, the concentration of the No. 3 tube is 125 pg/ml; and so on for gradient dilution to tube 7 (7.8 pg/ml). 500 pg/ml as the highest point of the standard curve, standard & sample & antibody diluent as the zero point (0 pg/ml) of the standard curve, that is, the blank value.

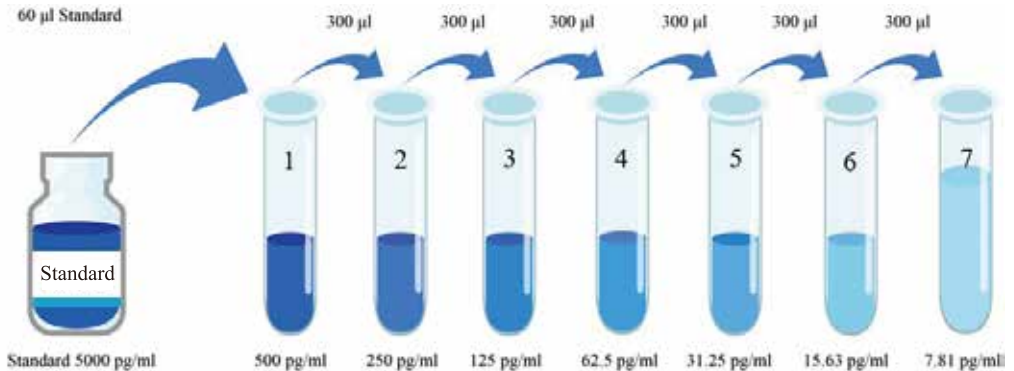

### Experimental Protocol

1. Bring all reagents to room temperature before use. Take out the plates required for the current experiment, put the unused plates in an aluminium foil pouch in time to reseal, and store them at 2~8°C.
2. Add the diluted standard and sample to wells of the plate respectively, and add standard & sample & antibody diluent to blank wells, 100  $\mu$ l/well. It is recommended that the standards and samples be tested in duplicate, and the order of adding reagents should be consistent so that the results of each duplicate well test are consistent.
3. Add 1 $\times$  detection antibody to each well, 50  $\mu$ l/well, shake on a microplate shaker for 30 seconds to mix well, cover with a sealing film, and incubate for 2 hours at room temperature.
4. Discard the liquid in the wells and wash wells with 1 $\times$  washing solution, 300  $\mu$ l/well. It is recommended to shake the plate on a microplate shaker for 30 seconds before washing, and then discard the washing solution. Repeat 5 times, the last time pat dry on a paper towel.
5. Add 1 $\times$  Streptavidin-HRP, 100  $\mu$ l/well, shake on a microplate shaker for 30 seconds to mix well, cover the plate with a plate sealer, and incubate for 30 minutes at room temperature.
6. Repeat Step 4.
7. Add TMB Chromogenic Substrate, 100  $\mu$ l/well, shake on a microplate shaker for 30 seconds to mix well, cover the plate with a plate sealer, and incubate for 20 minutes at room temperature.
8. After the incubation, add stop solution, 50  $\mu$ l/well, and read absorbance of the plate at the wavelength of 450 nm for the main wavelength and 620 nm for the reference wavelength.
9. After the experiment, put the unused reagents and the outer frame of the ELISA plate back into the kit and store them at 2~8°C. It is recommended to use up within 1 month.

### Sample Loading on The Microtiter Plate

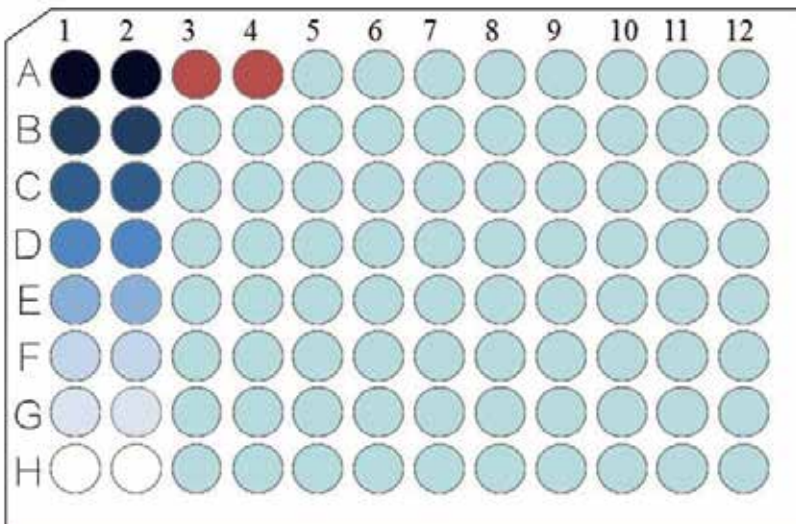

Notes: A1/A2: 100 µl 500 pg/ml Standard  
 B1/B2: 100 µl 250 pg/ml Standard  
 C1/C2: 100 µl 125 pg/ml Standard  
 D1/D2: 100 µl 62.5 pg/ml Standard  
 E1/E2: 100 µl 31.25 pg/ml Standard  
 F1/F2: 100 µl 15.63 pg/ml Standard  
 G1/G2: 100 µl 7.81 pg/ml Standard  
 H1/H2: 100 µl 0 pg/ml Standards (Standards & Samples & Antibody Diluents)  
 A3/A4: 100 µl Sample


### Result Analysis

1. Double-wavelength detection was performed with a microplate reader, and the OD values at the main wavelength of 450 nm and the reference wavelength of 620 nm were determined. The OD value is the OD measurement at 450 nm minus the OD measurement at 620 nm.
2. Calculate the average OD value of duplicate wells of the standard, then subtract the blank value (average OD value of the 0 pg/ml standard) to obtain the corrected value for the standard. Taking the concentration of the standard product as the abscissa and the OD correction value as the ordinate, the standard curve was generated by linear regression or the four-parameter method.
3. Calculate the sample concentration from the sample OD value and the standard curve equation. If the OD value of the sample is higher than the upper limit of the standard curve, it should be re-measured after appropriate dilution, and the corresponding dilution should be multiplied when calculating the concentration.

### Reference Data

A standard curve needs to be established with each assay, and the following data are only for demonstration purposes.

Standard (pg/ml)	OD Value		Average	Corrected
500	2.45	2.551	2.5005	2.468
250	1.238	1.338	1.288	1.2555
125	0.608	0.621	0.6145	0.582
62.5	0.305	0.343	0.324	0.2915
31.25	0.151	0.179	0.165	0.1325
15.63	0.09	0.106	0.098	0.0655
7.81	0.064	0.075	0.0695	0.037
0	0.032	0.033	0.0325	0

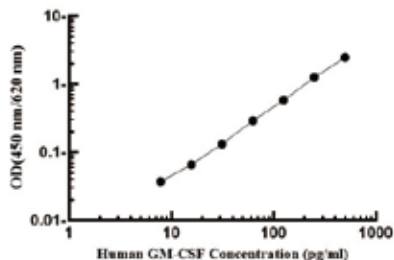

Interpretation of the results of the standard duplicate wells: In the above table, the average OD value of the two duplicate wells of the 0 pg/ml standard is  $(0.032+0.033)/2=0.0325$ , and the correction value is set as 0. The average OD value of the two duplicate wells of the 500 pg/ml standard is  $(2.45+2.551)/2=2.5005$ , and the corrected value is  $2.5005-0.0325=2.468$ .



## Precision

### Intra-assay Precision

Intra-assay precision was assessed by assaying 20 replicate wells on one microplate using 3 samples of known concentration.

### Inter-assay Precision

Inter-assay precision was assessed by assaying 20 replicate wells on different microplate with 3 samples of known concentration.

	Intra-assay			Inter-assay		
	1	2	3	1	2	3
Average (pg/ml)	198.4	93.3	44.4	200.3	95.7	43.8
Standard Deviation	8.4	3.4	1.2	6.9	3.8	1.8
Coefficient of Variation (%)	4.2	3.6	2.7	3.4	4.0	4.2

## Recovery Rate

Different concentrations of human GM-CSF were added to the serum, plasma and cell culture supernate of 4 healthy people, and the samples without GM-CSF were used as the background to calculate the recovery rate.

Sample	Average Recovery (%)	Range (%)
Serum	97	86~111
EDTA Plasma	98	84~117
Sodium Citrate Plasma	92	83~103
Heparin Plasma	95	87~105
Cell Supernate	99	91~110

## Linearity

High concentrations of human GM-CSF were added to the serum and plasma of 4 healthy people, and linear dilution was performed to detect the linear recovery rate.

Sample Dilution	Recovery Rate (%)	Serum	EDTA Plasma	Sodium Citrate Plasma	Heparin Plasma
1:2	Average (%)	108	102	120	95
	Range (%)	103~113	92~116	117~120	89~99
1:4	Average (%)	108	89	106	108
	Range (%)	81~119	85~97	94~112	100~113
1:8	Average (%)	111	99	113	101
	Range (%)	96~120	94~104	104~120	99~108

## Calibration

The standard of this kit is high-purity recombinant human GM-CSF calibrated by TransGen Biotech.

## Sensitivity

The lowest detectable concentration of human GM-CSF was 2 pg/ml. Sensitivity is the corresponding concentration calculated from the mean of 20 replicate zero standard OD values plus two standard deviations.



### Sample Value

The level of GM-CSF in 30 healthy human serum samples was detected by this kit, and the detection values of 30 samples were all lower than 7.8 pg/ml.

### Specificity

This kit recognizes native and recombinant human GM-CSF. Using recombinant human TNF- $\alpha$ , FGF-basic, IL-2, IL-12 p70, IL-6, IL-10, EGF, IFN- $\gamma$  and other cytokines for specific evaluation, no cross-reactivity and interference effects were observed.

### Notes

1. This kit should be stored at 2~8°C in the dark and used up within 1 month after opening.
2. To ensure accurate results, a standard curve is required for each assay.
3. All reagents used in the experiment should be thoroughly mixed.
4. After each plate washing, pat dry on a paper towel. If there are air bubbles in the plate wells, use a pipette tip to puncture them. Note that only one pipette tip can be used in each well to avoid cross-contamination.
5. TMB chromogenic substrate is a colorless and transparent liquid, please do not use it if there is discoloration.
6. After TMB develops color, it can be judged whether it is necessary to add a stop solution in advance or later according to the depth of color development.
7. After adding the stop solution, read within 30 minutes.
8. It is recommended to use the main wavelength of 450 nm and the reference wavelength of 620 nm for reading. If only a single wavelength of 450 nm is used for reading, the overall OD value may be high, and the blank value will also increase accordingly, resulting in a decrease in the accuracy of the kit.
9. Personal protective equipments are necessary in experiments for safety reasons. The stop solution in the kit is corrosive. Take care when using the reagent to avoid the risks. In case of accidental contact, please rinse with plenty of water and seek medical attention in time.
10. To avoid cross-contamination, use a new disposable pipette tips for each transfer. Please use disposable test tubes, pipette tips, plate sealers and clean plastic containers in the experiment.
11. Kit components from different batches or different sources cannot be used in combination.

**For research use only, not for clinical diagnosis.**

Version number: V1.0-202207

Service telephone +86-10-57815020

Service email [complaints@transgen.com](mailto:complaints@transgen.com)

